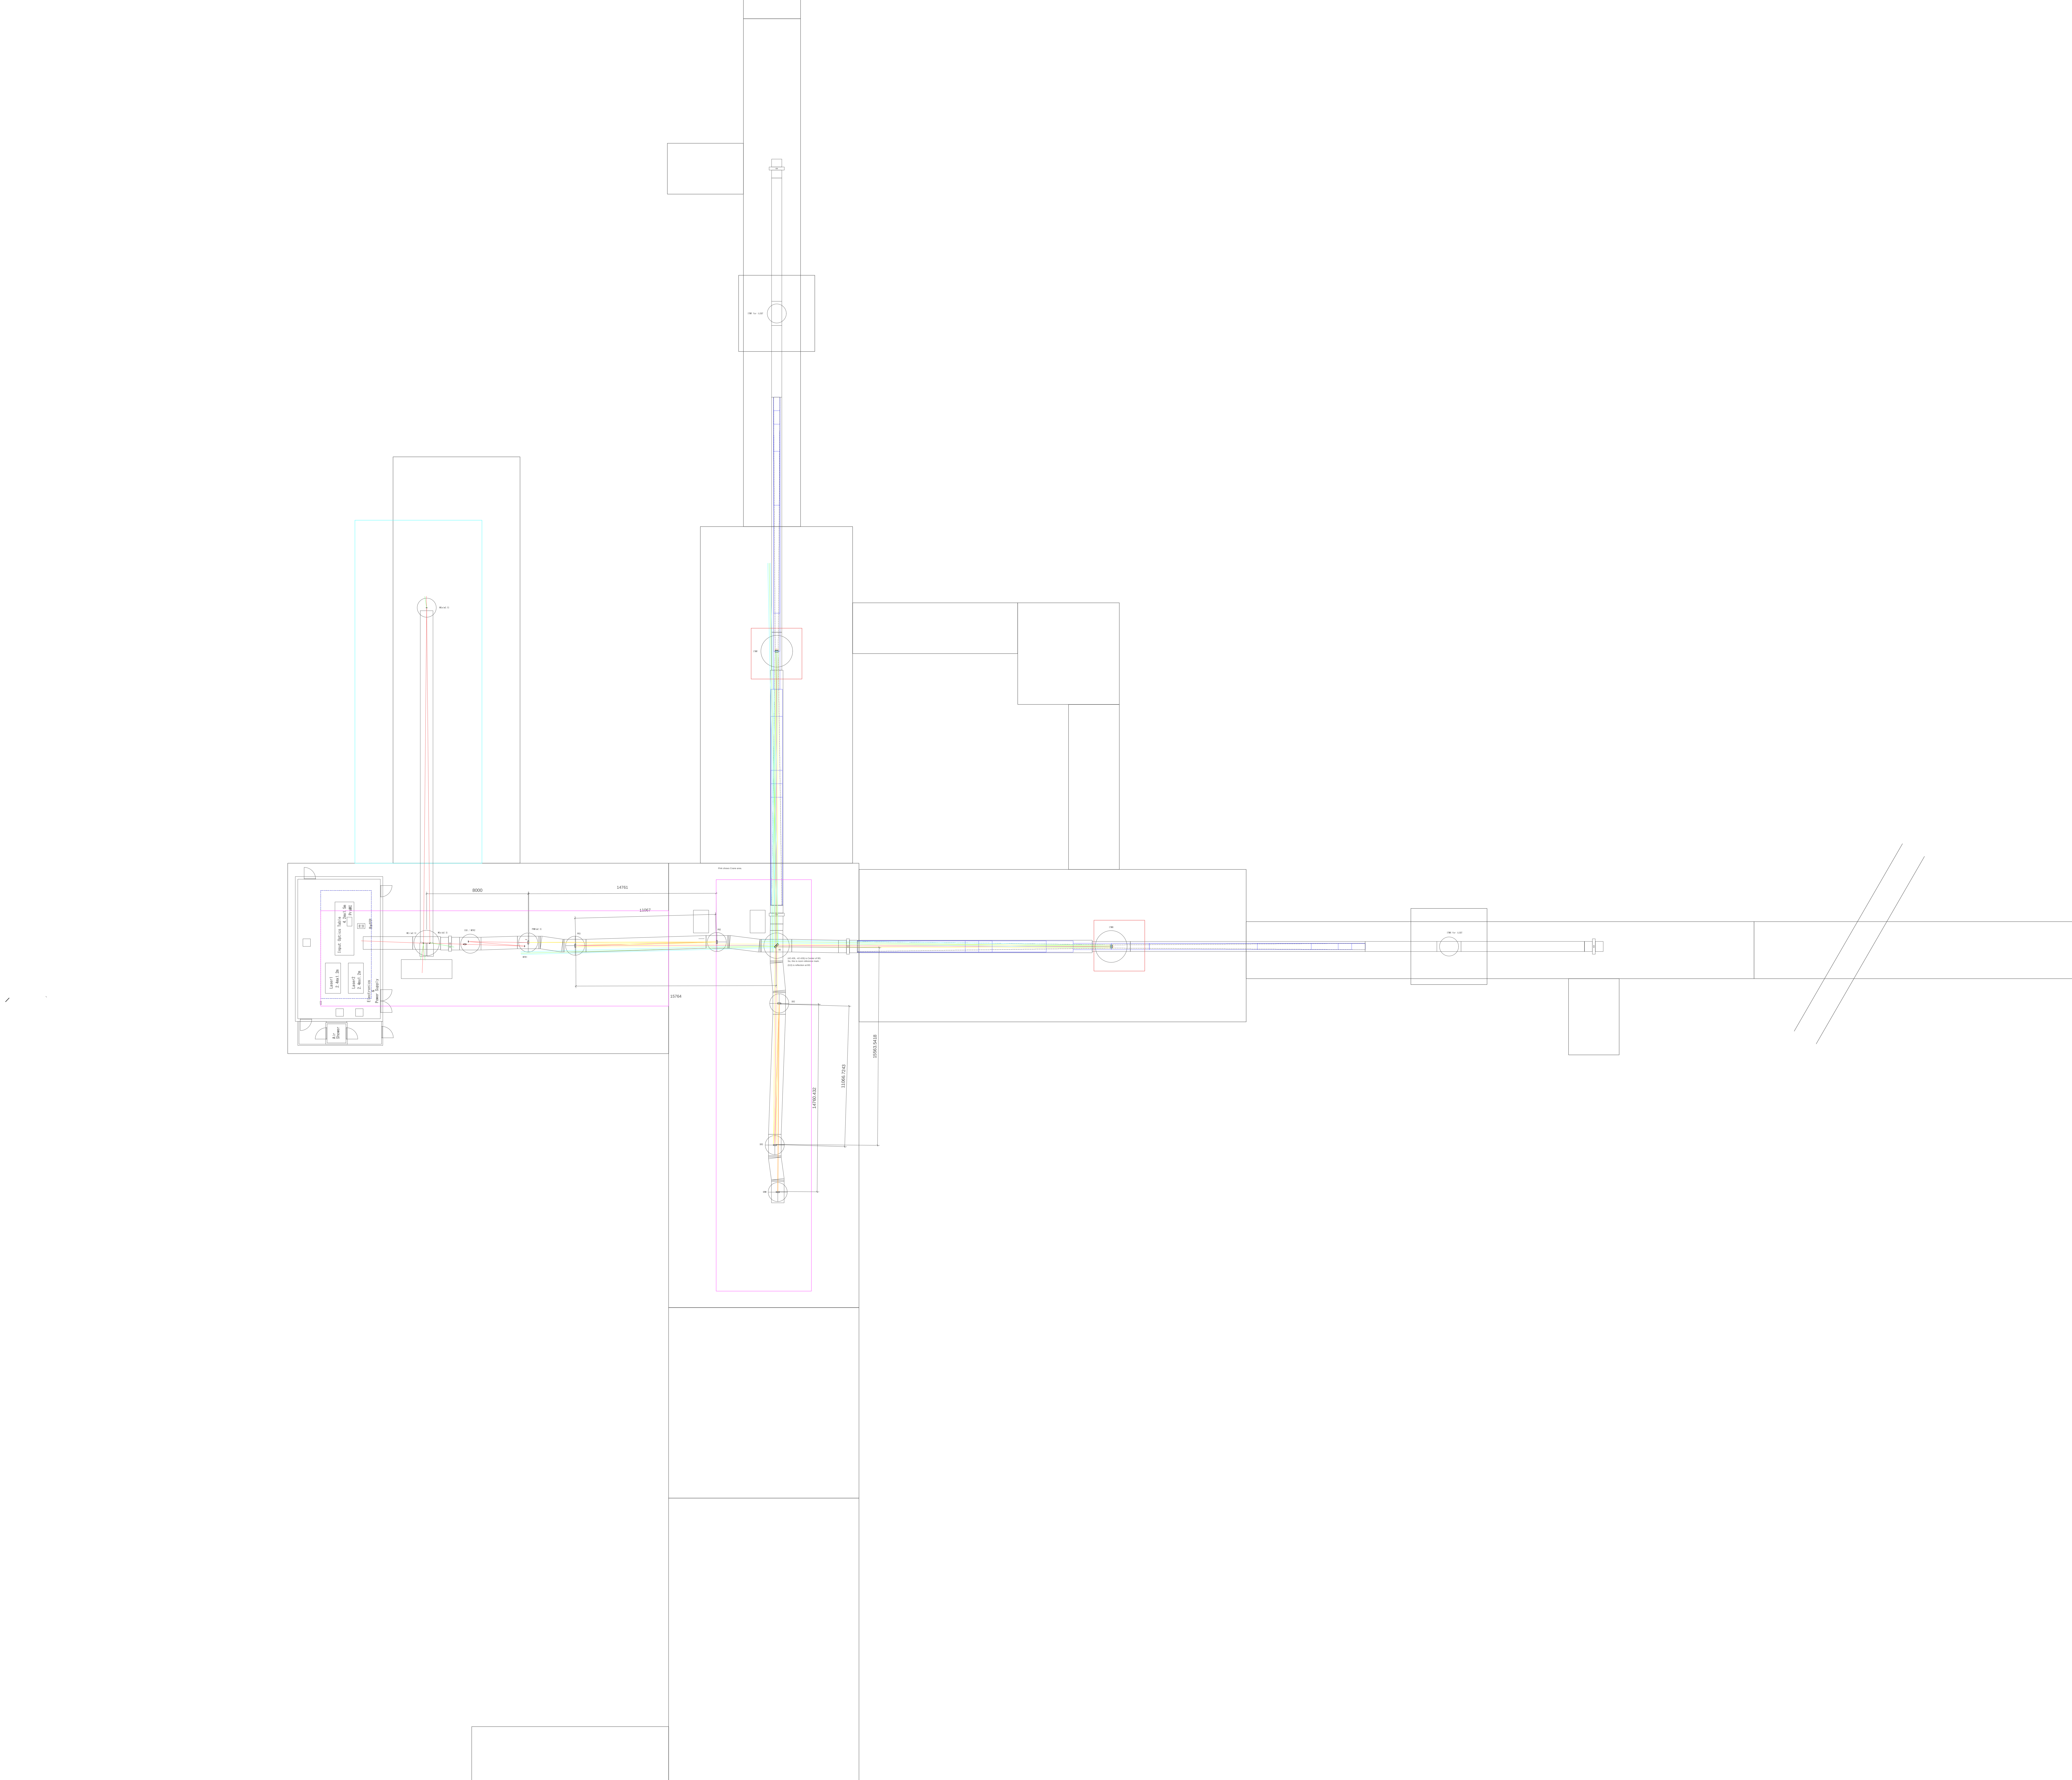
ITMY for iLCGT
MCe(w2.5)
ITMY
Pink shows Crane area.
8000
14761
11067
15764
Input Optics Table
4.2mx1.5m
PreMC
RefFP
Laser1
2.4mx1.2m
Laser2
2.4mx1.2m
Electronics
&
Power Supply
Air
Shower
MCi(w2.5)
MCo(w2.5)
ISO / MTR2
PRM(w2.5)
MTR1
PR3
PR2
BS
(42.426, -42.426) is Center of BS.
So, this is room reference mark.
(0,0) is reflection at BS
SR2
SR3
SRM
14760.432
11066.7243
15563.5418
ITMX
ITMX for iLCGT