

Interface Control Document of LCGT

Subgroup Name	Vibration Isolation System
Subgroup Leader	Ryutaro Takahashi National Astronomical Observatory of Japan
Sub-leader	Takashi Uchiyama Institute for Cosmic Ray Research
Sub-leader	Shinji Miyoki Institute for Cosmic Ray Research

Doc version	Date	Description
Rev. A-0	2009-05-28	Kick-off draft

APPROVAL AUTHORITIES

Concise definition of vibration isolation system

System requirement

Displacement of the test mass mirrors must be less than $6 \times 10^{-18} \text{m/Hz}^{1/2}$ at 5Hz where the seismic noise and the radiation pressure noise are crossed. RMS motion must be less than 0.1 μm . The test mass mirrors are cooled to 20K through heat links.

SAS

Core optics are suspended by SASs. Two kinds of SASs are used in LCGT. Type-A SAS consists of an IP, three stage MGAS filters and a cryogenic mirror suspension. Type-B SAS consists of an IP, two stage MGAS filters and a mirror suspension. Type-A SASs are used for FM1, FM2, EM1 and EM2. Type-B SASs are used for BS, PRM, SEM, MC2F and MC2E.

Stack

Three stage stacks are used for BS, PRM, SEM, MC2F, MC2E, MC1F, MC1E, MMT and PD. Rubbers are enclosed by welded bellows. Some optics are placed on the stage 0.

Glossary

SAS	Seismic Attenuation System
IP	Inverted Pendulum
MGAS	Monolithic Geometric Anti Spring
PF	Platform
IM	Intermediate Mass
MB	Magnet Box
TM	Test Mass
RM	Recoil Mass
ACC	Accelerometer
LVDT	Linear Variable Differential Transformer
FM	Front Mirror
EM	End Mirror
BS	Beam Splitter
PRM	Power Recycling Mirror
SEM	Signal Extraction Mirror
MC	Mode Cleaner
MMT	Mode Matching Telescope
PD	Photo Detector

Figure: Schematic drawing of the vibration isolation system.

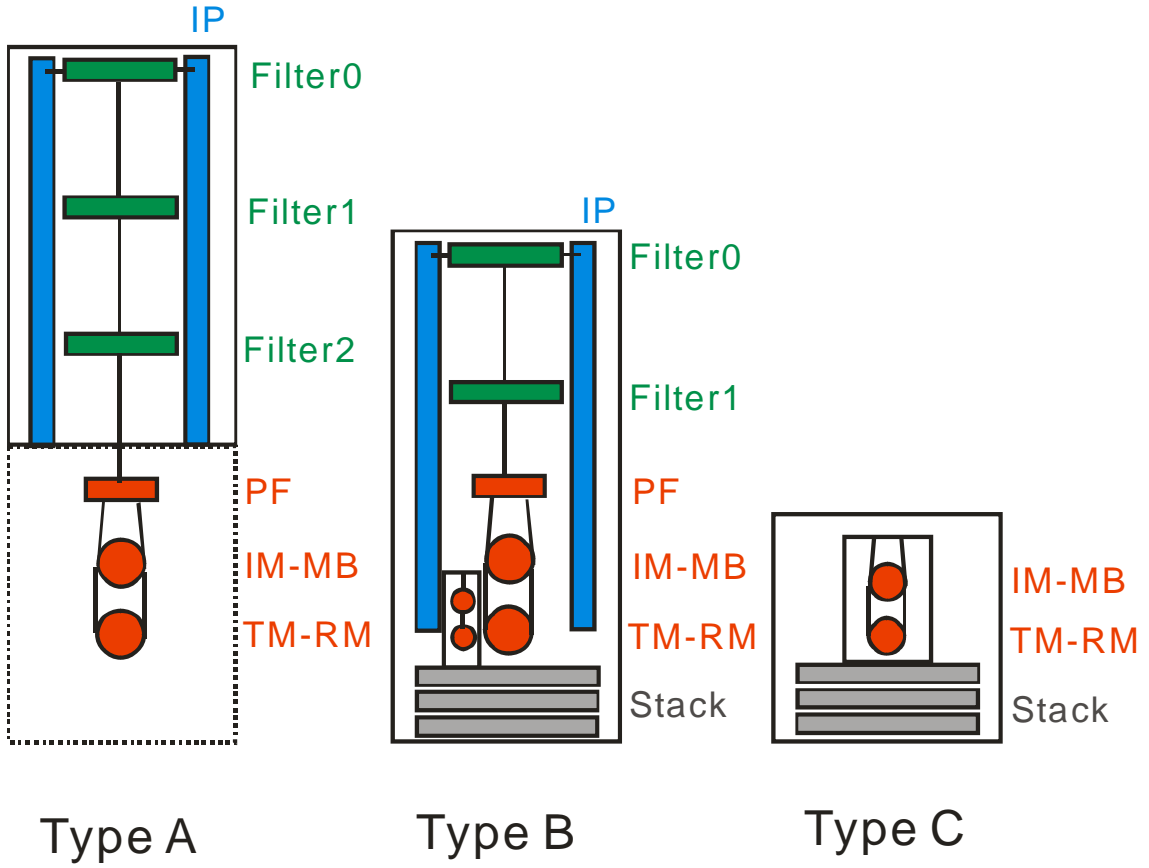


Table: Specification of the vibration isolation system

		#	Electric	Interface
Type-A SAS		4		Vacuum
Inverted pendulum (IP)	30mHz			
Leg		3		
ACC	$<10^{-10}$ m/Hz ^{1/2} @1Hz	3	DC15V	Control
LVDT	$<10^{-8}$ m/Hz ^{1/2} @1Hz	3	DC15V	Control
Actuator	10mm/V	3	DC15V	Control
Moter slider	?	3	?	Control
Filter0	H: 0.55Hz, V: 0.2Hz			
MGAS		1		
Picomoter		1	AC100V	Control
Filter1	H: 0.55Hz, V: 0.2Hz			
MGAS		1		
Filter2	H: 0.5Hz, V: 0.2Hz			
MGAS		1		
Platform (PF)	14K			
mini-GAS	V: 0.7Hz	4		
Picomoter		4	AC100V	Control
Actuator	1mm/V	8	DC15V	Control
Heat link	1W			Cryostat
Intermediate mass (IM)	15K			
Heat link	1W			Cryostat
Magnet block (MB)	14K			
Magnet	?	?		
Test mass (TM)	20K			Optics
Recoil mass (RM)	15K			
Actuator	?	4	DC15V	Control
Type-B SAS		5		Vacuum
Inverted pendulum (IP)	30mHz			
Leg		3		
ACC	$<10^{-10}$ m/Hz ^{1/2} @1Hz	3	DC15V	Control
LVDT	$<10^{-8}$ m/Hz ^{1/2} @1Hz	3	DC15V	Control
Actuator	10mm/V	3	DC15V	Control
Moter slider	?	3	?	Control
Filter0	H: 0.55Hz, V: 0.2Hz			
MGAS		1		
Picomoter		1	AC100V	Control
Filter1	H: 0.55Hz, V: 0.2Hz			
MGAS		1		
Platform (PF)				
mini-GAS	V: 2Hz	4		
Picomoter		4	AC100V	Control
Actuator	1mm/V	8	DC15V	Control
Intermediate mass (IM)				
Magnet block (MB)				
Magnet	?	?		
Test mass (TM)				Optics
Recoil mass (RM)				
Actuator	?	4	DC15V	Control

		#	Electric	Interface
Stack	2Hz	9		Vacuum
Stage 0				
Breadboard		1		
Bellows		3		
Rubber		3		
Stage 1				
Block		3		
Bellows		9		
Rubber		9		
Stage 2				
Block		3		
Bellows		9		
Rubber		9		